



Tooth preparation

- Make sure to create a stump with a 4° - 6° cone. Round off all the transitions within the preparation to avoid unwanted tension under the restoration material.
- Also make sure to avoid tangential, spring edge or lip preparations. Therefore, exercise special care when using instruments with a round tip and do not introduce them any further than up to half their diameter at maximum! Please note that tangential preparations are technically unfeasible and would result in too thin, i. e. instable and overcontoured, crown margins.
- The preparation limit must have a width of at least 1 mm.
- Both a shoulder preparation with rounded interior angles and a distinct chamfer preparation may be carried out. Rework the preparation margin using finishing instruments of matching shape.

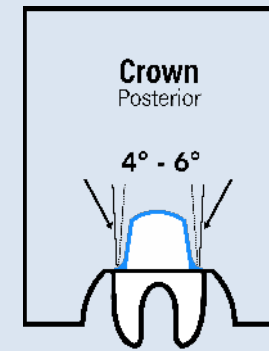


Model the workpiece on the computer

- Permanent crowns, inlays, onlays, veneers:
Always keep the minimum wall thickness – even after manual grinding
(The dimensions apply also to artificial teeth and temporary crowns, inlays, onlays and veneers)

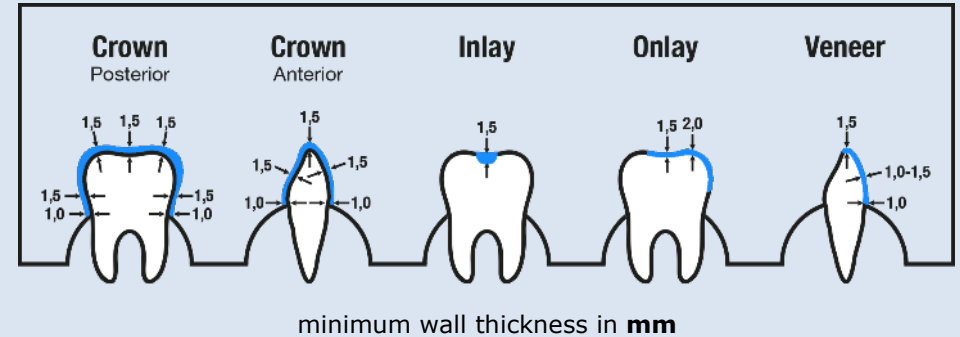

- Temporary bridges:
Keep a connector size of at least 16 mm²

The connector area should be as large as possible.
For physical stability, the height of the connector is more important than the width. Doubling the width results in only doubling the strength, while doubling the height results in eight times the strength. Oval connector areas are therefore recommended.

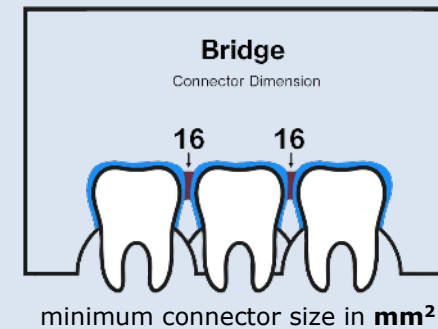

Generate the printing file

Use the appropriate software "Alpha 3D" and download the required parameter set from Ackuretta's database. Deliver it in a suitable form to the printer by observing the instruction for use of the software and of the printer.

Note

Ensure to use the appropriate version of the file!


<https://ackuretta.com/pages/alpha-3d>

Also make sure that you have selected the "Resin Type" menu with "saremco print CROWNTEC".

Useful hints

Create the supports on the occlusal surface.

With a 0.3 mm thick "Bounding Box" or also called "Base Plate" the material holds perfectly during printing and can easily be removed from the platform after printing.

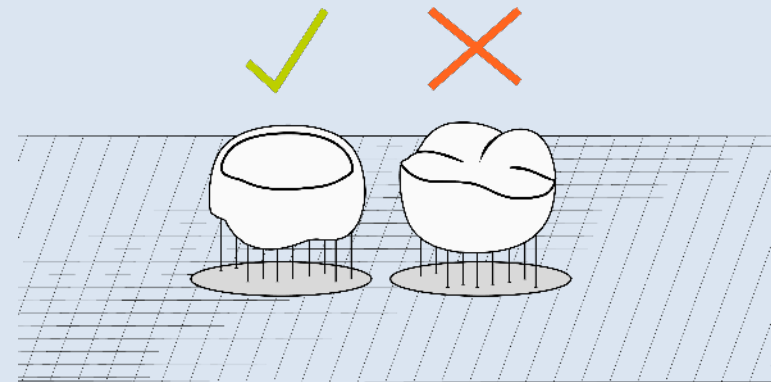

Print

- Work as clean as possible
- Dirty trays or machines can cause deformation/discoloration
- Briefly shake the resin (1 – 3 minutes) and pour it into the tray of the printer
- Start the printing process

Note

Wait until a printing temperature of 35° C / 95° F is reached.



- Remove the printed object carefully from the platform



- Roughly snap off the supports



- Remove excessive material with an alcohol-soaked (96 %) cloth or brush
- Clean the interdental areas and the interior surfaces of the crown with a suitable alcohol-soaked (96 %) brush, until the surface is lightly matt

Note

Never soak the printed job into alcohol.



Freshly printed

Surface: glossy
Inside: glossy



Not enough cleaned


Surface: slightly matt
Inside: glossy



well cleaned

Surface: slightly matt
Inside: slightly matt

- Dry thoroughly with an air syringe

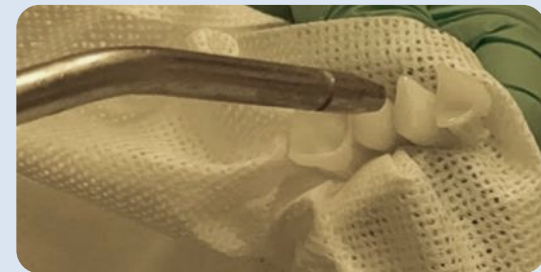


Optional step

Carefully sandblast the printed part surfaces to remove the remaining coating using a sandblaster with polish blasting material 50 µm at a maximum blasting pressure of 1.5 bar.

Note

Take care to avoid any deformation or damage of the printed job.

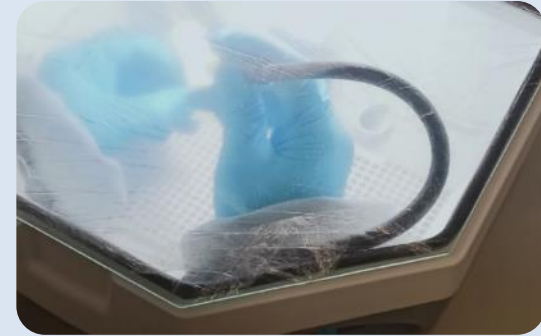

Optional step – Individualization of the crown or tooth

Apply intensive colors e.g. *els paintart* from SAREMCO.



Finish the printed job - Cure

- Polymerize in an appropriate UV-light box with a wavelength of 320 – 500nm. Suggestion: "Signum HiLite Power" from Haereus Kulzer (2 x 180 s) or UV-Flash device "Otoflash G171" from NK-Optik (2 x 2000 flashes; turn objects between the exposure cycles)
- Make sure that the light device performs still with the adequate light-power.

Note

To achieve the desired material properties, biocompatibility and final shade, post-curing of the completely dried and cleaned job is necessary.

Useful hint

Speed up the color finalization placing the printed job into boiling water (100 °C) for 2 minutes after post-curing.



Finish the printed job – Polish

- Work out the restoration with 40 μ and 12 μ diamond burs
- Polish to a high gloss using polishing brushes, polishing discs, strips or silicone polishers



Attach – permanent crowns, inlays, onlays or veneers to the tooth

- Roughen the inside of the printed object by sandblasting with an abrasive (Al_2O_3 , $110\mu m$)
- Then, fix it definitively with an appropriate composite cement material. Panavia V5. (Kuraray) and Variolink (Ivoclar) are recommended

Note

Zinc-phosphate cements as well as glass-ionomer-cements are only of limited suitability due to their opacity.



OR

Attach – temporary crowns, bridges, inlays, onlays or veneers to the tooth

Attach the finished temporary prosthesis with a commercially available provisional cement.



OR

Attach – artificial teeth on a denture base

- Roughen the base surface of the printed artificial teeth for e.g. by sandblasting (Al_2O_3 , $110\mu\text{m}$)



- Apply a primer and a bonding material, insert in the prosthesis according to the natural shape and polymerize

Alternatively, CROWNTEC can also be used directly as bonding material. Put a small amount of material with a brush on the roughened teeth-surface of the artificial tooth, put it into the prosthesis, eliminate any excess material and light-cure it from all sides for at least 20 seconds.



or

Attach – artificial teeth in a denture base (classical manufacturing)

Use a classical manufacturing procedure like the pouring method with cold cure resin after roughening the teeth.



https://de.wikipedia.org/wiki/Datei:Making_of_complete_denture_04.JPG#filelinks

SAREMCO Dental AG
Gewerbstrasse 4
CH-9445 Rebstein / Schweiz
Tel: +41 (0) 71 775 80 90
Fax: +41 (0) 71 775 80 99
info@saremco.ch
www.saremco.ch

Edited 12/2021 | D600238